

## **References**

1. Anatyuk L.I. (2003). *Termoelektrichestvo. Tom II. Termoelektricheskie preobrazovateli energii [Thermoelectricity. Vol.II. Thermoelectric power converters]*. Chernivtsi: Bukrek [in Russian].
2. Anatyuk L.I., Cherkez R.G. (2010). Permeable segmented thermoelement in electric power generation mode. *J. Thermoelectricity*, 3, 5-12.
3. Cherkez R. G. (2012). Energy possibilities of permeable generator thermoelements based on segmented legs. AIP Conf. Proc. 1449, 443, pp. 439-442; doi:<http://dx.doi.org/10.1063/1.4731590>
4. Pontryagin L.S., Boltianskiy V.G., Gamkrelidze R.F., Mishchenko. (1976). *Matematicheskaya teoriya optimalnykh protsessov [Mathematical theory of optimal processes]*. Moscow: Nauka [in Russian].
5. Bublik V.T., Drabkin I.A., Karataiev V.V., et al. (2012). Obimnyi nanostrukturirovannyi termoelektricheskii material na osnove (Bi,Sb)<sub>2</sub>Te<sub>3</sub>, poluchennyi metodom iskrovogo plasmennogo spekanii (SPS) [Bulk nanostructured thermoelectric material based on (Bi,Sb)<sub>2</sub>Te<sub>3</sub> obtained by spark

Submitted 03.07.2019

**L.I. Anatyhuk** *acad. National Academy of Sciences of Ukraine*<sup>1,2</sup>,  
**N.V. Pasechnikova** *doc. med. sciences, National Academy  
of medical sciences of Ukraine*<sup>3</sup>,  
**V.O. Naumenko** *doc. med. sciences*<sup>3</sup>,  
**O.S. Zadorozhnyi** *cand. med. sciences*<sup>3</sup>,  
**Nazaretian P.E.**<sup>3</sup>, **Havryliuk M.V.**<sup>1,2</sup>, **Tiumentsev V.A.**<sup>1</sup>,  
**R.R. Kobylanskyi** *cand. Phys.-math. sciences*<sup>1,2</sup>,

<sup>1</sup>Institute of Thermoelectricity of the NAS and MES of Ukraine,  
1, Nauky str., Chernivtsi, 58029, Ukraine;

<sup>2</sup>Yu.Fedkovych Chernivtsi National University,  
2, Kotsiubynskyi str., Chernivtsi, 58012, Ukraine

<sup>3</sup>State Institution “The Filatov Institute of Eye Diseases and  
Tissue Therapy of the NAMS of Ukraine”, Odesa, Ukraine

## **THERMOELECTRIC DEVICE FOR HYPOTHERMIA OF THE HUMAN EYE**

---

*The paper presents the results of the development of a thermoelectric device in the form of a monocular dressing for contact cooling of the human eye through the eyelids. The developed device allows controlled local contact cooling of the eye structures through the eyelids and is designed to treat the acute and chronic eye diseases, reduce intraocular pressure, and reduce pain and inflammatory processes of the eye. The design features of the device and its technical characteristics are presented. Bibl. 23, Fig. 2, table 1.*

**Key words:** thermoelectric device, thermoelectric cooling, hypothermia of the human eye.

### **Introduction**

Therapeutic hypothermia is a curative effect that involves reducing the patient's body temperature by forcing heat away from the surface of the body or internal organs to reduce the risk of ischemic tissue damage. Therapeutic hypothermia in medicine has been known for over 200 years as an effective and proven method of neuroprotection in patients with some critical conditions, which reduces the mortality of patients and reduces the amount of damage to brain tissue. Currently, therapeutic hypothermia is considered to be the most promising physical method of neuroprotective protection of the brain, since from the standpoint of evidence-based medicine there is no effective method of pharmacological neuroprotection in neuroresuscitation practice [1]. Therapeutic hypothermia is successfully used in various fields of medicine (cardiac surgery, neurosurgery, resuscitation, etc.) in order to increase the resistance of brain cells to ischemia [2-6].

It is known that cerebral metabolism changes with the temperature of the brain, on average by 6-8% when the temperature of the body changes by 1 °C [1]. Lowering the temperature of the neurons of the central nervous system causes the development of metabolic depression in them, which leads to a decrease in oxygen consumption, increased resistance to hypoxia, ischemia and reperfusion [7, 8]. In general, the following mechanisms of the neuroprotective action of therapeutic hypothermia are

currently distinguished: inhibition of destructive enzymatic reactions; inhibition of free radical reactions; plasticity protection of lipoproteins of cytoplasmic membranes; reduced oxygen consumption in areas of the brain with low blood flow; improving oxygen delivery to the ischemic zones of the brain and reducing intracranial pressure; inhibition of biosynthesis and production of excitotoxic neurotransmitters [9-12].

At the same time, it is known that general therapeutic hypothermia is accompanied by the risk of complications, so it can be applied only in specially equipped resuscitation units. In clinical conditions in an ophthalmic hospital, it is not justified due to the complexity of its implementation [3, 4]. In ophthalmology there is a prospect of using local therapeutic hypothermia, for example, to reduce intraocular pressure. According to some authors, this effect is achieved by reducing the production of intraocular fluid and improving the outflow of watery moisture.

In so doing, there is a decrease in pain syndrome [13 – 15]. There is evidence in the literature that local hypothermia of the eye can lead to a decrease in fibrin production, a decrease in bleeding volume, and a decrease in photodamage during surgery [16]. A number of authors demonstrate a decrease in choroidal blood flow and a decrease in damage to the hemato-retinal barrier in conditions of local hypothermia [17, 18]. There is evidence of the use of local hypothermia to reduce inflammatory reactions [19]. It is known that after local hypothermia significant hemodynamic changes occur in the eye that are characterized by a significant expansion of the vessels and a decrease in their peripheral resistance, leading to an increase in blood flow to the vascular tract, an increase in pulse volume and blood flow velocity [20].


There are various ways to cool the eyes. In the experiment, it was confirmed that with local contact hypothermia, a decrease in the temperature of the intraocular medium of the rabbit eye is possible, both by cooling directly the external surface of the cornea and when exposed to cold through closed eyelids [21]. To solve this problem, you can use, for example, a bubble with ice, laying it on the eyelids [14]. Another way to achieve local hypothermia is achieved by irrigating the outer surface of the eye with chilled solutions. During intraocular surgery, local hypothermia of the eye can be created by lowering the temperature of irrigation solutions [22]. With regard to modern technologies, the development of special thermoelectric devices for local contact eye cooling looks promising. This will allow more efficient and controlled use of the beneficial effects of therapeutic hypothermia for the treatment of ophthalmic diseases.

Therefore, *the purpose of this work* is to design and manufacture an experimental sample of thermoelectric device in the form of a monocular dressing for contact cooling of the human eye through the eyelids.

## **Device design and specifications**

At the Institute of Thermoelectricity of the NAS and MES of Ukraine within cooperation agreement with the State Institution "The Filatov Institute of Eye Diseases and Tissue Therapy of the NAMS of Ukraine" a thermoelectric device was developed in the form of a monocular dressing for contact cooling of the human eye through the eyelids (Fig.1). The technical characteristics of the device are given in Table 1.

The device is designed to treat acute and chronic eye diseases, reduce intraocular pressure, reduce pain and inflammation of the human eye. The developed thermoelectric medical device allows controlled local cooling of eye structures through the eyelids and makes it possible to develop and introduce the technology of controlled local therapeutic hypothermia in ophthalmology. This device is original and has no world analogues.

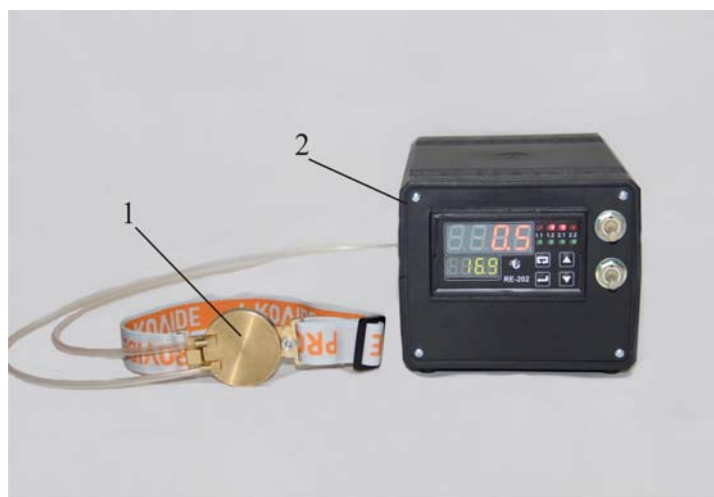

*Fig.1. Experimental sample of a thermoelectric device in the form of a monocular dressing for contact cooling of human eyes through the eyelids: 1 – cooling plate, 2 – thermoelectric electronic cooling, control and power supply unit*

*Table*

*Device specifications*

<b>№</b>	<b>Device specifications</b>	<b>Parameter values</b>
1.	Operating temperature range	(+5 ÷ +40) °C
2.	Temperature accuracy	± 0.2 °C
3.	Discreteness of the measured and set temperature	± 0.1 °C
4.	Temperature measurement error, not more	± 0.2 °C
5.	Thermal load in the external circuit, not more	20 W
6.	Total power consumption, not more	120 W
7.	Supply voltage (AC 50 Hz)	220 ± 10 V
8.	Overall dimensions of cooling plate	(75×45×12) mm
9.	Dimensions of thermoelectric electronic cooling, control and power supply unit	(180×120×100) mm
10.	Pump performance	40 l/h
11.	Length of hoses with external temperature sensor	1 m
12.	Device weight	1.5 kg
13.	Device run-up time	10 min
14.	Device continuous work time	48 h

The device consists of two main functional units: cooling plate 1 and thermoelectric electronic cooling, control and power supply unit 2 (Fig. 1). The cooling plate 1 is a liquid heat exchanger made of a


highly conductive material - copper. The electronic unit 2 comprises a thermoelectric cooling unit, a power supply unit and an electronic control unit based on a programmable thermoregulator of the type RE-202. In turn, the thermoelectric cooling unit contains a Peltier thermoelectric module [23, 24], liquid heat exchangers and a circulation pump.

The Peltier thermoelectric module is designed to cool or heat the liquid circulating in the outer circuit. The hot side of this thermoelectric module is cooled by an internal liquid circuit connected to the water supply network. The circulation pump provides for the circulation of the liquid coolant in the outer circuit.

The power supply unit is designed to power the thermoelectric module from an alternating current network of 220 V. The temperature regulator RE-202 measures the temperature from internal and external thermoresistive sensors and generates control signals for the control circuit. In turn, the control circuit controls the thermoelectric module according to a predetermined program in order to maintain the operating temperature set by the operator.

On the front panel of the device there are toggle switches "ON", "HEATING / COOL" and a digital display of the temperature regulator RE-202. The rear panel of the device accommodates a "NETWORK" toggle switch, a socket for connecting to a 220 V network, sockets for connecting external temperature sensors "T1" and "T2", "CIRCUIT INPUT", "CIRCUIT OUTPUT", "WATER INPUT", "WATER OUTPUT" unions and a 5 A fuse.

A block-diagram of the thermoelectric device for contact cooling of the human eye is shown in Fig.2, where 1 is a 220V network switch, 2 is a RE-202 measuring thermoregulator, 3 is a power supply unit switch, 4 is a power supply unit, 5 is a tank with the liquid of heat exchanger circuit, 6 is a temperature sensor of the object, 7 is a temperature sensor of heat exchanger circuit, 8 is a job type switch, 9 is a circulation pump, 10 is a working heat exchanger of liquid circuit, 11 is an active heat exchanger of liquid circuit, 12 is a thermoelectric Peltier module, 13 is a power relay of thermoelectric Peltier module; 14 is a passive heat exchanger of liquid circuit, 15 is water mains.

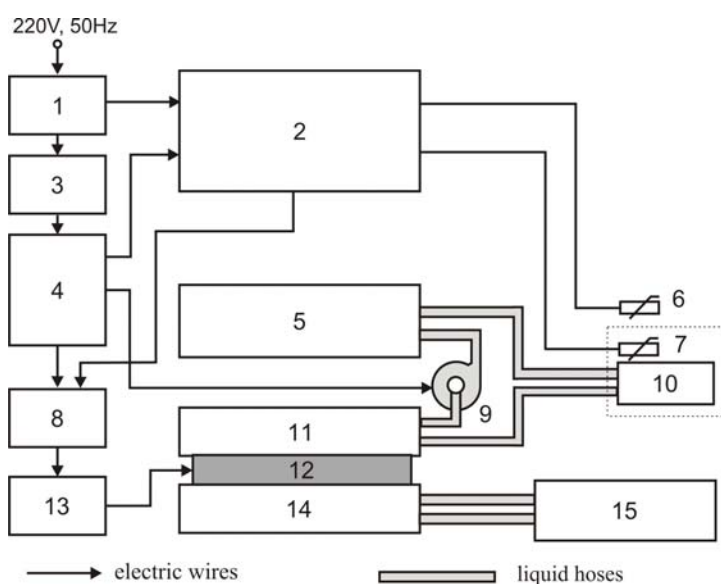

*Fig. 2. Block-diagram of a thermoelectric device in the form of a monocular dressing for contact cooling of the human eye through the eyelids: 1 – 220 V mains switch, 2 - measuring thermoregulator RE-202 3 –power supply switch, 4 – power supply unit, 5 – tank with a liquid of heat exchanger circuit, 6 – object temperature sensor, 7 – temperature sensor of heat exchanger circuit, 8 – job type switch, 9 – circulation pump, 10 – working heat exchanger of liquid circuit, 11 – active heat exchanger of liquid circuit, 12 – thermoelectric Peltier module, 13 – power relay of thermoelectric Peltier module, 14 –passive heat exchanger of liquid circuit, 15 – water mains.*

## **Operating principle of device**

The operating principle of device is cooling or heating (thermal stabilization) of the human eye in order to treat acute and chronic diseases of the eye, reduce intraocular pressure, reduce pain and inflammatory processes.

The proposed device works as follows. After electrical power supply and selection of cooling or heating mode, the thermoelectric module maintains the temperature set by the thermoregulator by means of liquid circulating in the circuit. If the internal temperature sensor is selected as the feedback sensor, the preset temperature in the liquid circuit stabilizes. If an external sensor is selected as the feedback sensor and it is located in a thermostatically controlled object, then the temperature of the object is stabilized.

The specified device is simple, compact, portable and reliable in operation, which allows a doctor or a medical person to use it without special training, having read the instruction in advance. Thus, the technical advantages of this device include: the presence of a highly efficient thermoelectric Peltier module, the ability to measure and maintain a set temperature with a discreteness of  $\pm 0.2$  °C, the safety of use of the device and the ability to monitor the temperature of the human eye surface in real time.

The introduction of such a device into medical practice will be of great social and economic importance as it will reduce the risk of ophthalmic complications, preserve the viability of patients' eye structures, and provide highly skilled care both in specialized medical establishments and in extreme conditions. This, in turn, will provide the right conditions for the preservation of human health, improve the efficiency and quality of health care delivery and make a significant contribution to the development of the newest domestic medical thermoelectric equipment.

It should be noted that in order to confirm the effectiveness of the device, the development of methods of treatment and clinical trials, the developed experimental model of the device for contact cooling of the human eye through the eyelids was submitted to the State Institution "The Filatov Institute of Eye Diseases and Tissue Therapy of the NAMS Ukraine" within cooperation agreement. The results of clinical trials of the device will be the subject of subsequent publications on this subject matter.

## **Conclusions**

1. For the first time, a design was developed and an experimental sample was made of a thermoelectric device in the form of a monocular dressing for contact cooling of human eyes through the eyelids. The device is designed to treat the acute and chronic eye diseases, reduce intraocular pressure, and reduce pain and inflammation of the human eye. The proposed device has no world analogues.
2. The developed thermoelectric medical device makes it possible to carry out controlled contact cooling of human eye structures in the temperature range ( $+5 \div +40$ ) °C and will further allow developing and introducing the technology of controlled local therapeutic hypothermia in ophthalmology.

## **References**

1. Tsarev A.V. (2014). Tselevoi temperaturnyi menedzhment v klinicheskoi praktike intensivnoi terapii kriticheskikh sostoianii [Targeted temperature management in the clinical practice of

- critical state intensive therapy]. *Meditsina neotlozhnykh sostoianii – Emergency Medicine*, 7, 186-191 [in Russian].
2. Alzaga A.G., Cerdan M., Varon J. (2006). Therapeutic hypothermia. *Resuscitation*, 70 (3), 369-380.
  3. Polderman K.H., Herold I. (2009). Therapeutic hypothermia and controlled normothermia in the ICU: Practical considerations, side effects, and cooling methods. *Crit. Care Med.*, 37, 1101-1120.
  4. Saad H., Aladawy M. (2013). Temperature management in cardiac surgery. *Glob. Cardiol. Sci. Pract.*, 1, 44-62.
  5. The hypothermia after cardiac arrest group. Mild therapeutic hypothermia to improve the neurologic outcome after cardiac arrest. (2002). *N. Engl. J. Med.*, 346, 549-556.
  6. Yenari M.A., Han H.S. (2012). Neuroprotective mechanisms of hypothermia in brain ischaemia. *Nat. Rev. Neurosci.*, 13, 267-278.
  7. Bernard S., Buist M. (2003). Induced hypothermia in critical care medicine: A review. *Critical Care Medicine*, 31, 2041-2051.
  8. Lampe J.W., Becker L.B. (2011). State of the art in therapeutic hypothermia. *Annu. Re. Med.*, 11, 104-10.
  9. Usenko L.V., Tsarev A.V. (2009). Iskusstvennaia hipotermiia v sovremennoi reanimatologii [Artificial hypothermia in modern resuscitation]. *Obshchaiia reanimatologiya – General Resuscitation*, 5(1), 21-23.
  10. Mayer S.A., Sessler V.A. (2005). *Therapeutic hypothermia*. New York: Marcel Dekker.
  11. Nunnally M.E., Jaeschke R., Bellingan G.J., et al. (2011). Targeted temperature management in critical care: A report and recommendations from five professional societies. *Critical Care Medicine*, 39, 1113-1125.
  12. Safar P. (2002). *Cerebral resuscitation from temporary complete global brain ischemia*. In: *Cerebral blood flow: mechanisms of ischemia, diagnosis, and therapy*. Pinsky M.R.(Ed.) Berlin: Springer.
  13. Chanchikov G.F., Zavolskaia Z.P., Bereznikova V.I. (1978). Vliianiie umerennoi lokalnoi hipotermii na ophtalmotonus, zritelnyie funktsii i gidrodinamiku glaz bolnykh glaukomoj [Influence of moderate local hypothermia on intralocular tension, visual functions and hydrodynamics of patients ill with glaucoma]. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 8, 594-597 [in Russian].
  14. Shif L.V., Taratynova A.V., Neiman V.A., Angelova N.V. (1981). Primeneniie lokalnoi gipotermii pri ostrom pristupe glaukomy i glaukome v terminalnoi stadii, oslozhnivsheisia bolevym sindromom [The use of local hypothermia in an acute attack of glaucoma and glaucoma in the terminal stage, complicated by pain]. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 3, 187-188 [in Russian].
  15. Tamai K., Majima A., Honda F. (1993). Experimental study on local cooling of the eyeball in ocular surgery. The local cooling effect on uveal blood circulation, intraocular pressure, and intravitreal pressure. *Nippon Ganka Gakkai Zasshi*, 97, 509–513.
  16. Jabbour N.M., Schepens C.L., Buzney S.M. (1998). Local ocular hypothermia in experimental intraocular surgery. *Ophthalmology*, 95, 1685-1690.
  17. Fujishima H., Yagi Y, Toda I., Shimazaki J., Tsuota K (1995). Increased comfort and decreased inflammation of the eye by cooling after cataract surgery. *Am. J. Ophthalmol.*, 119, 301–306.

18. Tamai K., Toumoto E., Majima A. (1997). Local hypothermia protects the retina from ischaemic injury in vitrectomy. *Br J. Ophthalmol.*, 81, 789-794.
19. Zolotareva M.M., Chvialeva K.I., Vasilevich A.I. (1978). *Gipotermiia pri glaznykh zabolivaniakh [Hypothermia with eye diseases]*. Minsk [in Russian].
20. Lazarenko V.I., Chanchikov G.F., Kornilovskii I.M., Gaidabura V.G. (1976). Vliianiie umerennoi lokalnoi hipotermii na hemo- i hidrodinamicheskiye pokazateli zdorovykh glaz [Influence of moderate local hypothermia on the hemo-and hydrodynamic parameters of healthy eyes]. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 6, 419-422 [in Russian].
21. Zadorozhnyi O.S., Nazaretian R.E., Mirnenko V.V., Naumenko V.A., Pasechnikova N.V. (2018). *Eksperymentalnoie issledovaniie epibulbarnoi i intraokuliarnoi temperatury krolika v usloviakh hipotermii [Experimental study of epibulbar and intraocular temperature of rabbit under hypothermia]*. *Oftalmologiya. Vostochnaia Evropa - Ophthalmology. Eastern Europe*, 1, 73-81.
22. Anatyshuk L.I., Pasechnikova N.V., Naumenko V.A., Nazaretian R.E., Umanets N.N., Kobylianskyi R.R., Zadorozhnyi O.S. (2019). Dynamics of intraocular temperature in the process of vitreoretinal surgery using irrigational solutions of various temperature. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 1, 33-38 [in Russian].
23. Anatyshuk L.I. (1979). *Termoelementy i termoelektricheskiye ustroystva. Spravochnik (Thermoelements and thermoelectric devices. Handbook)*. Kyiv: Naukova Dumka [in Russian].  
Anatyshuk L.I. (2003). *Termoelektrichestvo. T.2. Termoelektricheskiye preobrazovateli energii [Thermoelectricity. Vol.2. Thermoelectric power converters]*. Kyiv-Chernivtsi: Institute of Thermoelectricity [in Russian].

Submitted 10.07.2019

**Анатишук Л.І. акад. НАН України,<sup>1,2</sup>**  
**Пасєчнікова Н.В. док. мед.– наук, НАМН України,<sup>3</sup>**  
**Кобилянський Р.Р. канд. фіз.– мат. наук<sup>1,2</sup>,**  
**Науменко В.О.<sup>3</sup>, Задорожний О.С. канд. мед.– наук<sup>3</sup>,**  
**Гаврилюк М.В.<sup>1,2</sup>, Тюменцев В.А.<sup>1</sup>**

<sup>1</sup>Інститут термоелектрики НАН і МОН України,  
вул. Науки, 1, Чернівці, 58029, Україна,  
*e-mail: anatysh@gmail.com;*

<sup>2</sup>Чернівецький національний університет імені Юрія Федьковича,  
вул. Коцюбинського 2, Чернівці, 58012, Україна,  
<sup>3</sup>ДУ «Інститут очних хвороб і тканинної терапії  
ім. В.П. Філатова НАМН України», Французький  
бульвар, 49/51, Одеса, 65061, Україна,  
*e-mail: zadoroleg2@gmail.com.*

**ТЕРМОЕЛЕКТРИЧНИЙ ПРИЛАД ДЛЯ  
ГІПОТЕРМІЇ ОКА ЛЮДИНИ**



У роботі наведено результати розробки термоелектричного приладу у вигляді монокулярної пов'язки для контактної охолодження ока людини через повіки. Розроблений прилад дає можливість контрольованого локального контактної охолодження структур ока через повіки та призначений для лікування гострих і хронічних захворювань ока, зниження внутрішньоочного тиску, зменшення больового синдрому та запальних процесів ока. Наведено особливості конструкції приладу та його технічні характеристики. Бібл. 23, рис. 2, табл. 1.

**Ключові слова:** термоелектричний прилад, термоелектричне охолодження, гіпотермія ока людини.

**Анатичук Л.І.** ак. НАН України,<sup>1,2</sup>  
**Пасєчнікова Н.В.** доктор мед. наук, НАМН України,<sup>3</sup>  
**Кобиланський Р.Р.** канд. фіз.-мат. наук<sup>1,2</sup>,  
**Науменко В.О.**<sup>3</sup>, **Задорожний О.С.** канд. мед. наук<sup>3</sup>,  
**Гаврилюк М.В.**<sup>1,2</sup>, **Тюменцев В.А.**<sup>1</sup>

<sup>1</sup>Інститут термоелектричності НАН і МОН України, ул. Науки, 1,  
Черновці, 58029, Україна, e-mail: anatysh@gmail.com;

<sup>2</sup>Черновицький національний університет  
ім. Юрія Федьковича, ул. Коцюбинського, 2,  
Черновці, 58012, Україна

<sup>3</sup>ДУ «Інститут глазних захворювань і тканинної терапії  
ім. В.П. Філатова НАМН України», Французький  
бульвар, 49/51, Одеса, 65061, Україна,  
e-mail: zadoroleg2@gmail.com.

## ТЕРМОЕЛЕКТРИЧЕСКИЙ ПРИБОР ДЛЯ ГИПОТЕРМИИ ОКА ЧЕЛОВЕКА

В работе приведены результаты разработки термоэлектрического устройства в виде монокулярной повязки для контактной охлаждения глаза человека через веки. Разработанный прибор дает возможность контролируемого локального контактного охлаждения структур глаза через веки и предназначен для лечения острых и хронических заболеваний глаза, снижение внутриглазного давления, уменьшение болевого синдрома и воспалительных процессов глаза. Приведены особенности конструкции прибора и его технические характеристики. Библ. 23, рис. 2, табл. 1.

**Ключевые слова:** термоэлектрический прибор, термоэлектрическое охлаждение, гипотермия глаза человека.

### References

1. Tsarev A.V. (2014). Tselevoi temperaturnyi menedzhment v klinicheskoi praktike intensivnoi terapii kriticheskikh sostoianii [Targeted temperature management in the clinical practice of

- critical state intensive therapy]. *Meditina neotlozhnykh sostoianii – Emergency Medicine*, 7, 186-191 [in Russian].
2. Alzaga A.G., Cerdan M., Varon J. (2006). Therapeutic hypothermia. *Resuscitation*, 70 (3), 369-380.
  3. Polderman K.H., Herold I. (2009). Therapeutic hypothermia and controlled normothermia in the ICU: Practical considerations, side effects, and cooling methods. *Crit. Care Med.*, 37, 1101-1120.
  4. Saad H., Aladawy M. (2013). Temperature management in cardiac surgery. *Glob. Cardiol. Sci. Pract.*, 1, 44-62.
  5. The hypothermia after cardiac arrest group. Mild therapeutic hypothermia to improve the neurologic outcome after cardiac arrest. (2002). *N. Engl. J. Med.*, 346, 549-556.
  6. Yenari M.A., Han H.S. (2012). Neuroprotective mechanisms of hypothermia in brain ischaemia. *Nat. Rev. Neurosci.*, 13, 267-278.
  7. Bernard S., Buist M. (2003). Induced hypothermia in critical care medicine: A review. *Critical Care Medicine*, 31, 2041-2051.
  8. Lampe J.W., Becker L.B. (2011). State of the art in therapeutic hypothermia. *Annu. Re. Med.*, 11, 104-10.
  9. Usenko L.V., Tsarev A.V. (2009). Iskusstvennaia hipotermiia v sovremennoi reanimatologii [Artificial hypothermia in modern resuscitation]. *Obshchaaia reanimatologiya – General Resuscitation*, 5(1), 21-23.
  10. Mayer S.A., Sessler V.A. (2005). *Therapeutic hypothermia*. New York: Marcel Dekker.
  11. Nunnally M.E., Jaeschke R., Bellingan G.J., et al. (2011). Targeted temperature management in critical care: A report and recommendations from five professional societies. *Critical Care Medicine*, 39, 1113-1125.
  12. Safar P. (2002). *Cerebral resuscitation from temporary complete global brain ischemia*. In: *Cerebral blood flow: mechanisms of ischemia, diagnosis, and therapy*. Pinsky M.R.(Ed.) Berlin: Springer.
  13. Chanchikov G.F., Zavolskaia Z.P., Bereznikova V.I. (1978). Vliianiie umerennoi lokalnoi hipotermii na ophtalmotonus, zritelnyie funktsii i gidrodinamiku glaz bolnykh glaukomoii [Influence of moderate local hypothermia on intralocular tension, visual functions and hydrodynamics of patients ill with glaucoma]. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 8, 594-597 [in Russian].
  14. Shif L.V., Taratynova A.V., Neiman V.A., Angelova N.V. (1981). Primeneniie lokalnoi gipotermii pri ostrom pristupe glaukomy i glaukome v terminalnoi stadii, oslozhnivsheisia bolevym sindromom [The use of local hypothermia in an acute attack of glaucoma and glaucoma in the terminal stage, complicated by pain]. *Oftalmologicheskii Zhurnal - J. Ophthalmology*, 3, 187-188 [in Russian].
  15. Tamai K., Majima A., Honda F. (1993). Experimental study on local cooling of the eyeball in ocular surgery. The local cooling effect on uveal blood circulation, intraocular pressure, and intravitreous pressure. *Nippon Ganka Gakkai Zasshi*, 97, 509–513.
  16. Jabbour N.M., Schepens C.L., Buzney S.M. (1998). Local ocular hypothermia in experimental intraocular surgery. *Ophthalmology*, 95, 1685-1690.
  17. Fujishima H., Yagi Y, Toda I., Shimazaki J., Tsuota K (1995). Increased comfort and decreased inflammation of the eye by cooling after cataract surgery. *Am. J. Ophthalmol.*, 119, 301-306.
  18. Tamai K., Toumoto E., Majima A. (1997). Local hypothermia protects the retina from